

SLS ISO 5636 PART 6: 2018
(ISO 5636-6: 2015)
UDC 621.798

**PAPER AND BOARD - DETERMINATION
OF AIR PERMEANCE (MEDIUM RANGE)
PART 6: OKEN METHOD**

SRI LANKA STANDARDS INSTITUTION

Sri Lanka Standard
PAPER AND BOARD -- DETERMINATION OF AIR PERMEANCE
(MEDIUM RANGE)
PART 6: OKEN METHOD

SLS ISO 5636 PART 6: 2018
(ISO 5636-6: 2015)

Gr. G

Copyright Reserved
SRI LANKA STANDARDS INSTITUTION
17, Victoria Place
Elvitigala Mawatha
Colombo - 08
Sri Lanka.

Sri Lanka Standards are subject to periodical revision in order to accommodate the progress made by industry. Suggestions for improvement will be recorded and brought to the notice of the Committees to which the revisions are entrusted.

This Standard does not purport to include all the necessary provisions of a contract

© ISO 2015 - All right reserved.

© SLSI 2018

All right reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the SLSI.

Sri Lanka Standard
PAPER AND BOARD -- DETERMINATION OF AIR PERMEANCE
(MEDIUM RANGE)
PART 6: OKEN METHOD

NATIONAL FOREWORD

This Standard was approved by the Sectoral Committee on Paper, Board and Packaging and was authorized for adoption and publication as a Sri Lanka Standard by the Council of the Sri Lanka Standards Institution on 2018-08-10

The text of the International Standard **ISO 5636-6: 2015** Paper and board- Determination of air permeance (medium range) - Part 6: Oken method has been accepted for adoption as a Sri Lanka Standard which specifies the Oken method for determining the air permeance or air resistance of papers and boards.

This Sri Lanka Standard is identical with **ISO 5636-6: 2015** Paper and board- Determination of air permeance (medium range) - Part 6: Oken method published by the International Organization for Standardization (ISO).

TERMINOLOGY AND CONVENTIONS

The text of the International Standard has been accepted as suitable for publication, without deviation, as a Sri Lanka Standard. However, certain terminology and conventions are not identical with those used in Sri Lanka Standards. Attention is therefore drawn to the following:

- a) Wherever the words “International Standard” appear referring to a particular Standards they should be interpreted as “Sri Lanka Standard”.
- b) The comma has been used throughout as a decimal marker. In Sri Lanka Standards it is the current practice to use the full point at the base as the decimal marker.
- c) Wherever page numbers are quoted, they are ISO page numbers.

Cross References

International Standard

Corresponding Sri Lanka Standard

ISO 48, Rubber, vulcanized or thermoplastic — Determination of hardness (hardness between 10 IRHD and 100 IRHD)

SLS 297 Method of testing vulcanized rubber - Part 4- Determination of hardness (hardness between 10 IRHD and 100 IRHD)

ISO 186, Paper and board — Sampling to determine average quality

No corresponding Sri Lanka Standard

ISO 187, Paper, board and pulps — Standard atmosphere for conditioning and testing and procedure for monitoring the atmosphere and conditioning of samples

No corresponding Sri Lanka Standard

.....

**Paper and board — Determination of
air permeance (medium range) —**

**Part 6:
Oken method**

*Papier et carton — Détermination de la perméabilité à l'air (plage de
valeurs moyennes) —*

Partie 6: Méthode Oken





COPYRIGHT PROTECTED DOCUMENT

© ISO 2015, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

	Page
Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	1
5 Apparatus	2
5.1 Air resistance apparatus (Oken tester)	2
5.2 Water column type	2
5.3 Electronic sensor type	4
6 Sampling	5
7 Conditioning	5
8 Preparation of test pieces	5
9 Calibration	5
10 Procedure	5
11 Expression of results	6
11.1 Calculation of air permeance	6
11.2 Reporting the results	6
11.3 Standard deviation and coefficient of variation	6
12 Test report	6
Annex A (informative) Measurement principle of air resistance (Oken) and its relation to air resistance (Gurley)	8
Annex B (informative) Precision data	11
Bibliography	13

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 6, *Paper, board and pulps*, Subcommittee SC 2, *Test methods and quality specifications for paper and board*.

ISO 5636 consists of the following parts, under the general title *Paper and board — Determination of air permeance (medium range)*:

- *Part 3: Bendtsen method*
- *Part 4: Sheffield method*
- *Part 5: Gurley method*
- *Part 6: Oken method*

NOTE 1 *Part 1: General method* will be withdrawn after parts 3, 4, and 5 have been revised and published, as it was considered redundant.

NOTE 2 *Part 2: Schopper method* was withdrawn in 2006 as it was considered obsolete.

Paper and board — Determination of air permeance (medium range) —

Part 6: Oken method

1 Scope

This part of ISO 5636 specifies the Oken method for determining the air permeance and air resistance of paper and board. There is no limitation on the measuring range of air permeance or air resistance of papers and boards. It is unsuitable for rough-surfaced materials, which cannot be securely clamped to avoid leakage.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 48, *Rubber, vulcanized or thermoplastic — Determination of hardness (hardness between 10 IRHD and 100 IRHD)*

ISO 186, *Paper and board — Sampling to determine average quality*

ISO 187, *Paper, board and pulps — Standard atmosphere for conditioning and testing and procedure for monitoring the atmosphere and conditioning of samples*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

air permeance

mean air flow rate through unit area under unit pressure difference in unit time, under specified conditions

Note 1 to entry: Air permeance is expressed in micrometres per pascal second [$1 \text{ ml}/(\text{m}^2\text{Pa} \cdot \text{s}) = 1 \mu\text{m}/(\text{Pa} \cdot \text{s})$].

Note 2 to entry: This property is called air permeance and not air permeability because it is reported as a sheet property and is not normalized with respect to thickness to give a material property per unit thickness.

3.2

air resistance

time required for a specific volume of air under unit pressure to pass through unit area

Note 1 to entry: Air resistance is expressed in seconds per 100 millilitres (s/100 ml).

4 Principle

A test piece is clamped between a circular gasket and an annular flat surface of known dimensions. The absolute pressure on one side of the test piece is equivalent to atmospheric pressure. The air pressure on the inlet side of a narrow capillary of controlled dimensions is maintained at a constant value above

atmospheric pressure. The air passes through the capillary and then the test piece. The air pressure between the capillary and test piece depends on the permeance of the test piece. It is measured and converted to air permeance.

5 Apparatus

5.1 Air resistance apparatus (Oken tester)

Use either the water column type described in [5.2](#) or the electronic sensor type described in [5.3](#).

5.2 Water column type

5.2.1 The water column type (see [Figure 1](#)), consists of an air compressor ([5.2.1.2](#)), filter water column regulator ([5.2.1.3](#)), capillary ([5.2.1.3](#)), water column manometer ([5.2.1.4](#)), measuring head ([5.2.1.1](#)), and scale plate ([5.2.1.4](#)).

5.2.1.1 The measuring head, consists of clamping plates and a rubber gasket. The clamping plates are at the base of the apparatus and connected to the pressure measuring chamber by a tube. The equipment shall have a means of tightening the clamping plates together which might be a capstan (jackscrew) arrangement or a pneumatic system. The recommended clamping force is (180 ± 30) N. This mechanism provides a technique to give uniform loading and thus minimize the operator influence on the test. A controlled clamping force is the preferred method of clamping the test piece.

A rubber gasket is inserted concentrically into a groove in the upper surface of the lower clamping plate to prevent leakage of air between the surface of the paper and the clamping plate. The gasket consists of a thin, elastic, non-oxidizing material, having a smooth surface, rectangular cross section, a thickness of 1,5 mm to 2,0 mm, and a hardness of (50 ± 10) IRHD (international rubber hardness degrees) in accordance with ISO 48. The inside diameter of the gasket is $(28,3 \pm 0,3)$ mm and the outside diameter is $(34,5 \pm 0,5)$ mm.

The aperture of the gasket is concentrically aligned with the aperture in the clamping plates. To align and protect the gasket in use, it is cemented to a groove machined in the lower clamping plate. The groove is concentric with the aperture in the opposing plate, has an internal diameter of $(28,60 \pm 0,15)$ mm and an outside diameter of $(35,5 \pm 0,5)$ mm. The depth of the groove with a square bottom shall be $(0,5 \pm 0,1)$ mm less than the thickness of the gasket when mounted. The gasket, when mounted inside the concentric groove, defines the measurement area (642 mm^2 area). The gasket should be changed at regular intervals.

5.2.1.2 The air compressor and regulator, supply compressed and filtered air. The air is controlled to approximately 10 kPa by the air regulator.


5.2.1.3 The filter water column regulator and capillary, provide a constant pressure. The filter water column regulator consists of a water tank with an internal diameter of approximately 100 mm and a height of approximately 700 mm and a constant pressure chamber with a side tube. The open end of the side tube is $(500 \pm 0,5)$ mm below the water surface.

The air at approximately 10 kPa introduced into the constant pressure chamber is controlled to $(4,90 \pm 0,01)$ kPa [(500 ± 1) mmH₂O] and transferred to the pressure measuring chamber through the capillary.

The capillary consists of a narrow tube made of stainless material with an inner diameter of approximately 0,4 mm and a length of approximately 54 mm. The capillary length shall be strictly adjusted so that the time required for the passage of 100 ml of air through the capillary under a pressure difference of 1,23 kPa is equal to 100 s (see [A.2](#) for adjustment of the capillary length).

5.2.1.4 The water column manometer and scale plate, comprise the pressure measurement system. The water column manometer is connected to the water tank at a depth greater than 500 mm below the surface of the water in the water tank by a pipe with a diameter large enough (with a minimum of 3 mm) to allow water to transfer smoothly between the manometer and water tank. The manometer is connected to the measuring head and capillary. The scale plate for reading air resistance is marked in the units of seconds per 100 millilitres. The scale shall cover the range 0 s to 5 000 s with a scale reading of 0 at a pressure drop of zero (0 mmH₂O), a scale reading of 100 s/100 ml at the midpoint 250 mm below the surface level in the tank and infinity (∞) at a pressure of 4,90 kPa (500 mmH₂O).

NOTE High or low air resistance types of Oken tester with different capillary dimensions or measurement areas are available for shorter measurement time or higher precision. However, these types of Oken tester are out of the scope of this part of ISO 5636.

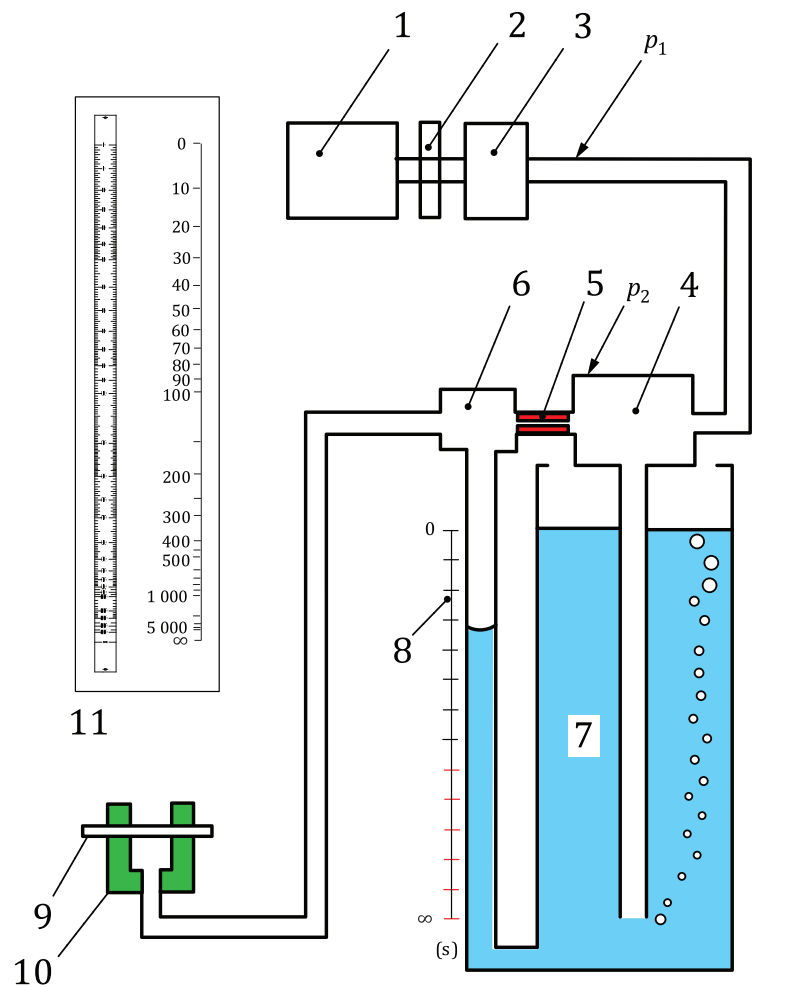

Key

- | | | | |
|---|---|-------|------------------------|
| 1 | air compressor | 8 | scale plate |
| 2 | filter | 9 | test piece |
| 3 | regulator | 10 | measuring head |
| 4 | filter water column regulator/constant pressure chamber | 11 | example of scale plate |
| 5 | capillary | p_1 | approximately 10 kPa |
| 6 | water column manometer/pressure measuring chamber | p_2 | 4,90 kPa |
| 7 | water tank | | |

Figure 1 — Diagram of water column type Oken tester

5.3 Electronic sensor type


5.3.1 The electronic sensor type (see [Figure 2](#)), consists of a measuring head ([5.3.1.1](#)), air compressor ([5.3.1.2](#)), filter, regulator ([5.3.1.2](#)), capillary ([5.3.1.3](#)), pressure sensor ([5.3.1.4](#)), sensor amplifier ([5.3.1.4](#)), and digital display ([5.3.1.4](#)).

5.3.1.1 The measuring head, consists of clamping plates and a rubber gasket. The structure is the same as the measuring head ([5.2.1.1](#)) for the water column type.

5.3.1.2 The air compressor and regulator, are the same as the air supply system ([5.2.1.2](#)). The regulator controls air directly to $(4,90 \pm 0,01)$ kPa [(500 ± 1) mmH₂O].

5.3.1.3 The constant pressure chamber and capillary, are the same as those for the water column type ([5.2.1.3](#)). Air at the pressure controlled by the regulator is transferred to the measuring head through the capillary.

5.3.1.4 The pressure measuring chamber, electronic pressure sensor, amplifier, and digital display, comprise the electronic sensing system. The digital display shows the pressure of the pressure measuring chamber and the air resistance calculated from the pressure (see [A.3](#)), as units of kiloPascal (mmH₂O) and second per 100 millilitres.

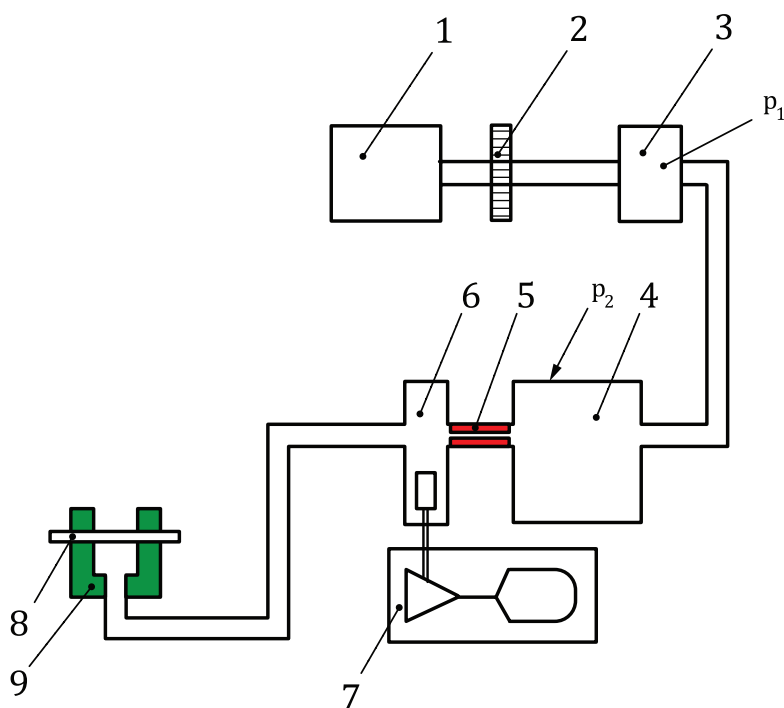

Key

- | | | | |
|---|---|-------|---------------------------|
| 1 | air compressor | 7 | amplifier/digital display |
| 2 | filter | 8 | test piece |
| 3 | regulator | 9 | measuring head |
| 4 | constant pressure chamber | p_1 | approximately 10 kPa |
| 5 | capillary | p_2 | 4,90 kPa |
| 6 | pressure measuring chamber/electronic pressure sensor | | |

Figure 2 — Diagram of electronic sensor type Oken tester

6 Sampling

If the mean quality of a lot is to be determined, sampling shall be in accordance with ISO 186. If the tests are made on another type of sample, make sure that the test pieces taken are representative of the sample received.

7 Conditioning

Condition the sample in accordance with ISO 187.

8 Preparation of test pieces

Prepare the test pieces in the same atmospheric conditions as those used to condition the sample.

Cut not less than 10 test pieces and identify their two sides, for example, side 1 and side 2. The test area shall be free from folds, wrinkles, holes, watermarks, or defects not inherent in the sample. Do not handle the part of the test piece which will become part of the test area. An adequate test piece size is 100 mm × 100 mm.

If the mean air permeance measured on the two sides is significantly different and if this difference is required to be shown in the test report, 10 tests are required for each side.

9 Calibration

Calibrate the apparatus according to instructions of the manufacturer.

Check the pressure of the water column manometer or digitally displayed pressure with no test piece between the clamping plates. It should be reading zero ($0 \pm 0,01$) kPa [(0 ± 1) mmH₂O]. If the water level does not read zero, adjust the water level by pouring water into the water tank. Check the apparatus for air leakage by clamping a thin sheet of smooth, rigid, impermeable material. The pressure shall be reading a value higher than 4,88 kPa (498 mmH₂O). If the value is less than the specified pressure, suggesting air leakage, check possible defects in the clamping plates, rubber gasket, and tubes to be repaired or replaced with new ones.

10 Procedure

Carry out the test in the same atmospheric conditions as those used to condition the samples.

Tests shall be performed according to the instructions of the manufacturer.

After the calibration process in [Clause 9](#), test a minimum of 10 test pieces, five with side 1 up and five with side 1 down.

Clamp a test piece between the clamping plates. Read the air resistance value of the water column manometer or digital display after the indication becomes stable.

Repeat the procedure until five valid measurements are obtained for each side.

Obtain the mean value of the 10 tests and also for the two sides separately.

If the mean air permeance measured on the two sides is significantly different (more than 10 %) and if this difference is required to be shown in the test report, 10 tests are required for each side.

11 Expression of results

11.1 Calculation of air permeance

Calculate the air permeance, P , in micrometres per pascal second, to two significant figures, from Formula (1):

$$P = \frac{127}{t_k} \quad (1)$$

where

t_k is the mean value of the air resistance in seconds by the Oken tester.

Formula (1) is based on a mean pressure difference between 0 and 4,90 kPa depending on the measured value and a test area of 642 mm².

NOTE 1 The coefficient of Formula (1) for the Oken tester is different from that for the Gurley apparatus because the calibration is based on 100 ml of air, at room pressure, passing through the test piece measured at a pressure difference of 1,23 kPa, which was specified in ISO 5636-5:1986.

NOTE 2 Air resistance (Oken) can be converted to air resistance (Gurley) using the conversion formula given in [Annex A](#).

If required, calculate the mean air permeance for each side separately.

11.2 Reporting the results

Report the air permeance to two significant figures.

If the air resistance is required, this shall be reported as “Air resistance (Oken)” in seconds that corresponds to t_k defined in [11.1](#). Report the air resistance to two significant figures.

11.3 Standard deviation and coefficient of variation

If the standard deviation or coefficient of variation is required, first calculate the individual air permeance for each test piece and from them, the standard deviation and coefficient of variation.

If the results for the two sides of the samples are reported separately, calculate the standard deviations or coefficients of variation for the two sides separately.

12 Test report

The test report shall include the following information:

- a) a reference to this part of ISO 5636, i.e. ISO 5636-6;
- b) the date and place of testing;
- c) all the information necessary for complete identification of the sample;
- d) the conditioning atmosphere used;
- e) the number of test pieces tested, as specified in [Clause 10](#) and [11.1](#);
- f) the type of Oken tester used;
- g) the mean air permeance or permeances, as specified in [11.2](#);
- h) if required, the air resistance or air resistances, as specified in [11.1](#);

- i) if required, the standard deviation or coefficient of variation or the values for each side, as specified in [11.3](#);
- j) any deviation from the specified procedure which might have affected the result.

Annex A (informative)

Measurement principle of air resistance (Oken) and its relation to air resistance (Gurley)

The principle for the calculation of air resistance (Oken) from the measured pressure to graduate the scale plate or display air resistance digitally and the formula for conversion from air resistance (Oken) to air resistance (Gurley) will be described below.

A.1 Definitions of air resistance (Gurley) and air resistance (Oken)

Before ISO 5636 was established, the Gurley tester was supposed to be designed to measure air resistance (Gurley) t_G , that is, time in seconds required for the volume $V_G = 100$ ml of air, measured at room pressure, under the pressure difference $p_G = 1,29$ kPa to pass through a test area of 642 mm² of a test piece.

In ISO 5636-5:1986, air resistance (Gurley) t_{G1986} was redefined as time required for the volume $V_G = 100$ ml of air under the pressure difference $p_{G1986} = 1,23$ kPa to pass through the test area.

The Oken tester is designed or calibrated according to the definition of ISO 5636-5:1986 assuming that air behaves as a laminar flow. In ISO 5636-5:2003, air resistance (Gurley) t_{G2003} was redefined again now as time required for the volume $V_G = 106$ ml of air under the pressure difference $p_{G2003} = 1,22$ kPa to pass through it. However, for the same test piece, the measured air resistance (Gurley) (s) has been the same value through the ISO revisions because the tester design was unchanged. In short, although it seemed that t_G or t_{G1986} was measured, whereas in practice, it was t_{G2003} that was measured.

The conversion formula from the measured pressure p to air resistance (Oken), t_K , is determined following the definition of t_{G1986} . Therefore, air resistance (Oken), t_K , is equal to air resistance (Gurley) t_{G1986} , namely, $t_K = t_{G1986}$, by definition and not equal to t_G or t_{G2003} .

A.2 Adjustment of the capillary length of the Oken tester

The air flow rate Q (ml/s) through the capillary from the constant pressure chamber at the pressure p_c to the pressure measurement chamber at a pressure p is equal to the air flow rate through the specimen, also expressed as Q (ml/s), when the relevant air volume is measured at room pressure (See [Figures 1](#) and [2](#)). A rate of laminar air flow would be proportional to the pressure difference and Formulae (A.1) and (A.2) apply.

$$Q = k_c (p_c - p) \quad (\text{A.1})$$

$$Q = k_s p \quad (\text{A.2})$$

where

k_c and k_s are the coefficient of air flowability [ml/(s kPa)] of the capillary and the test piece, respectively. k_s is assumed to be specific to the test piece, and not dependent on the pressure p .

For air resistance (Gurley) t_{G1986} and air flow rate Q_{G1986} (ml/s) in the Gurley condition specified in 1986 (1,23 kPa and 100 ml),

$$Q_{G1986} = k_s p_{G1986} \quad (\text{A.3})$$

$$t_{G1986} = \frac{V_{G1986}}{Q_{G1986}} = \frac{100}{k_s p_{G1986}} \quad (\text{A.4})$$

When Formula (A.1) and subsequently Formula (A.2) are substituted into Formula (A.4), Formula (A.5) is obtained.

$$t_{G1986} = \frac{100p}{Q p_{G1986}} = \frac{100p}{k_c (P_c - p) p_{G1986}} = \frac{100}{k_c p_{G1986}} \frac{p}{p_c - p} = K_{G1986} \frac{p}{p_c - p} \quad (\text{A.5})$$

where

$$K_{G1986} = \frac{100}{k_c p_{G1986}} \quad (\text{A.6})$$

For the Oken tester, the scale is graduated so that $t_K = 100$, namely, $t_{G1986} = 100$ at $P = 0,5p_c$. In this condition, Formula (A.5) leads to $K_{G1986} = 100$ and Formula (A.6) leads to

$$k_c = \frac{1}{p_{G1986}} \quad (\text{A.7})$$

This means that the capillary length shall be adjusted so that k_c satisfies Formula (A.7). In this case, $p = 0$ and Formula (A.1) become $Q = k_c p_c$. By definition, the time, t (s), required for the passage of 100 ml of air is such that $t = \frac{100}{Q} = \frac{100}{k_c p_c}$ and when this relationship is substituted into Formula (A.7), Formula (A.8) is obtained.

$$t = 100 \frac{p_{G1986}}{p_c} \quad (\text{A.8})$$

Therefore, the capillary length should be adjusted so that $t = 25,1$ s, which is calculated by substituting $p_{G1986} = 1,23$ kPa and $p_c = 4,90$ kPa into Formula (A.8).

A.3 Graduation of air resistance (Oken) from the measured pressure

If the relationship between pressure difference p and air resistance (Oken), t_K , is known, graduation on the scale plate or digital display of t_K will become possible. This relationship is $t_K = t_{G1986} = K_{G1986} \frac{p}{p_c - p}$ as shown by Formula (A.5). If a pressure difference p is expressed in water surface depth in the water column manometer, $p_c = 500$ mmH₂O (equivalent to 4,90 kPa). $K = 100$ is adopted for the Oken tester. Therefore, the conversion formula $t_K = \frac{100p}{500 - p}$ applies. For example, a water surface depth of 300 mmH₂O corresponds to $t_K = 100 \times 300 / (500 - 300) = 150$ (s).

A.4 Conversion from air resistance (Oken) to air resistance (Gurley) and air permeance

If the definition of t_{G2003} is represented like Formulae (A.3) to (A.6), Formulae (A.9) to (A.11) are obtained as follows:

$$Q_{G2003} = k_s p_{G2003} \quad (\text{A.9})$$

$$t_{G2003} = \frac{V_{G2003}}{Q_{G2003}} = \frac{106}{k_s p_{G2003}} \quad (\text{A.10})$$

$$t_{G2003} = \frac{106p}{Qp_{G2003}} = \frac{106p}{k_c(P_c - P)p_{G2003}} = \frac{106}{k_c p_{G2003}} \frac{p}{P_c - p} = K_{G2003} \frac{p}{P_c - p} \quad (\text{A.11})$$

where

$$K_{G2003} = \frac{106}{k_c p_{G2003}} \quad (\text{A.12})$$

The formula of conversion from air resistance (Oken), t_K , to air resistance (Gurley) t_{G2003} is obtained by the following process. For a test piece of air flowability k_s , air resistances measured with the two testers are from Formulae (A.4) and (A.10), $t_{G1986} = \frac{100}{k_s p_{G1986}}$ and $t_{G2003} = \frac{106}{k_s p_{G2003}}$, respectively. These two

formulae are combined and give

$$t_{G2003} = \frac{106 t_{G1986} p_{G1986}}{100 p_{G2003}} \quad (\text{A.13})$$

If $p_{G1986} = 1,23$ kPa and $p_{G2003} = 1,22$ kPa are substituted into Formula (A.12), Formula (A.14) is obtained.

$$t_{G2003} = \frac{106 \times 1,23}{100 \times 1,22} t_{G1986} = 1,07 t_{G1986} = 1,07 t_K \quad (\text{A.14})$$

Formula (A.14) is the conversion formula.

To calculate air permeance P [ml/(m²·Pa·s)] from air resistance (Oken), t_K , Formula (A.15) is applied.

$$P = \frac{100}{A p_{G1986} t_K} = \frac{100}{0,000\ 642 \times 1,23 \times 1\ 000 \times t_K} = \frac{127}{t_K} \quad (\text{A.15})$$

Note that this formula is different from the formula for air resistance (Gurley) t_{G2003} which is

$$P = \frac{106}{A p_{G2003} t_{G2003}} = \frac{106}{0,000\ 642 \times 1,22 \times 1\ 000 \times t_{G2003}} = \frac{135,3}{t_{G2003}} \quad (\text{A.16})$$

Annex B (informative)

Precision data

The precision data presented in [Tables B.1](#) and [B.2](#) have been obtained from JTAPPI-TSC, the testing standard committee of Japan TAPPI. The estimates of repeatability and reproducibility are based on data from the JTAPPI-TSC interlaboratory program in 2012. The materials on which these data are based were various grades of paper and board with a broad range of air resistance as listed in the tables. Only participants that were judged as acceptable by the interlaboratory analysis were included. The precision estimates are based on 10 determinations per test result and one test result per lab, per material.

The tests were conducted according to ISO/TR 24498[2] and TAPPI T 1200.[3]

The repeatability standard deviation reported in [Table B.1](#) is the “pooled” repeatability standard deviation, that is, the standard deviation is calculated as the root-mean-square of the standard deviations of the participating laboratories. This differs from the conventional definition of repeatability in ISO 5725-1.[4]

The repeatability and reproducibility limits reported are estimates of the maximum difference which should be expected in 19 of 20 instances when comparing two test results for material similar to those described under similar test conditions. These estimates might not be valid for different materials or different test conditions.

Repeatability and reproducibility limits are calculated by multiplying the repeatability and reproducibility standard deviations by 2,77.

NOTE 1 The repeatability standard deviation and the within-laboratory standard deviation are identical. However, the reproducibility standard deviation is not the same as between-laboratories standard deviation. The reproducibility standard deviation includes both the between-laboratories standard deviation and the standard deviation within a laboratory, viz.:

$$s_{\text{repeatability}}^2 = s_{\text{within lab}}^2 \quad \text{but} \quad s_{\text{repeatability}}^2 = s_{\text{within lab}}^2 + s_{\text{between lab}}^2$$

NOTE 2 $2,77 = 1,96 \times \sqrt{2}$, provided that the test results have a normal distribution and that the standard deviation, s , is based on a large number of tests.

Table B.1 — Estimation of repeatability of the test method from JTAPPI-TSC

Sample	Number of laboratories	Mean value	Repeatability standard deviation	Coefficient of variation	Repeatability limit
			s_r	$C_{V,r}$	r
		s	s	%	s
Coated paper	9	15 000	580	10,9	1 600
Coated board	9	5 100	120	6,6	340
Matte-coated paper	9	2 600	62	6,5	170
Light-weight coated paper	9	820	33	11,2	92
Uncoated board	9	230	18	20,9	48,5
Uncoated fine paper	7 ^a	22	1,7	21,8	4,8

^a Outliers not included.

Table B.2 — Estimation of the reproducibility of the test method from JTAPPI-TSC

Sample	Number of laboratories	Mean value <i>s</i>	Reproducibility standard deviation	Coefficient of variation	Reproducibility limit
			<i>s_R</i> <i>s</i>	<i>C_{V,R}</i> %	<i>R</i> <i>s</i>
Coated paper	9	15 000	910	17,3	2 500
Coated board	9	5 100	280	15,2	770
Matte-coated paper	9	2 600	110	12,1	320
Light-weight coated paper	9	820	47	15,9	130
Uncoated board	9	230	35	42,2	98
Uncoated fine paper	7 ^a	22	2,9	36,9	8,2

^a Outliers not included.

Bibliography

- [1] ISO 5636-5, *Paper and board — Determination of air permeance (medium range) — Part 5: Gurley method*
- [2] ISO 5725-1:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions*
- [3] ISO/TR 24498:2006, *Paper, board and pulps — Estimation of uncertainty for test methods*
- [4] TAPPI Test method T 1200 sp-07, *Interlaboratory evaluation of test methods to determine TAPPI repeatability and reproducibility*
- [5] KANO T. A Comparison between Oken Air Resistance-Smoothness Tester and Related Testers in Relation to Measured Values. Japan TAPPI Journal. 2008, **62** (12) p. 84
- [6] YAMAMOTO K., IWASAKI A., MIYAGI Z., IWASAKI M., HARA S. Development of a New Permeability Tester of Paper. Journal of Precision Engineering, Japan. 1985, **51** (4) p. 861

SLS CERTIFICATION MARK

The Sri Lanka Standards Institution is the owner of the registered certification mark shown below. Beneath the mark, the number of the Sri Lanka Standard relevant to the product is indicated. This mark may be used only by those who have obtained permits under the SLS certification marks scheme. The presence of this mark on or in relation to a product conveys the assurance that they have been produced to comply with the requirements of the relevant Sri Lanka Standard under a well designed system of quality control inspection and testing operated by the manufacturer and supervised by the SLSI which includes surveillance inspection of the factory, testing of both factory and market samples.

Further particulars of the terms and conditions of the permit may be obtained from the Sri Lanka Standards Institution, 17, Victoria Place, Elvitigala Mawatha, Colombo 08.



SRI LANKA STANDARDS INSTITUTION

The Sri Lanka Standards Institution (SLSI) is the National Standards Organization of Sri Lanka established under the Sri Lanka Standards Institution Act No. 6 of 1984 which repealed and replaced the Bureau of Ceylon Standards Act No. 38 of 1964. The Institution functions under the Ministry of Science & Technology.

The principal objects of the Institution as set out in the Act are to prepare standards and promote their adoption, to provide facilities for examination and testing of products, to operate a Certification Marks Scheme, to certify the quality of products meant for local consumption or exports and to promote standardization and quality control by educational, consultancy and research activity.

The Institution is financed by Government grants, and by the income from the sale of its publications and other services offered for Industry and Business Sector. Financial and administrative control is vested in a Council appointed in accordance with the provisions of the Act.

The development and formulation of National Standards is carried out by Technical Experts and representatives of other interest groups, assisted by the permanent officers of the Institution. These Technical Committees are appointed under the purview of the Sectoral Committees which in turn are appointed by the Council. The Sectoral Committees give the final Technical approval for the Draft National Standards prior to the approval by the Council of the SLSI.

All members of the Technical and Sectoral Committees render their services in an honorary capacity. In this process the Institution endeavours to ensure adequate representation of all view points.

In the International field the Institution represents Sri Lanka in the International Organization for Standardization (ISO), and participates in such fields of standardization as are of special interest to Sri Lanka.