

SRI LANKA STANDARD 1287: 2022
(ISO 976:2013)
UDC 678.8

**METHOD OF TESTING FOR
RUBBER AND PLASTICS FOR
POLYMER DISPERSIONS AND RUBBER
LATICES — DETERMINATION OF pH**
(First Revision)

SRI LANKA STANDARDS INSTITUTION

Sri Lanka Standard
METHOD OF TESTING FOR RUBBER AND PLASTICS FOR POLYMER
DISPERSIONS AND RUBBER LATICES — DETERMINATION OF pH
(First Revision)

SLS 1287: 2022
(ISO 976:2013)

Gr. E

Copyright Reserved
SRI LANKA STANDARDS INSTITUTION
17, Victoria Place
Elvitigala Mawatha
Colombo - 08
Sri Lanka.

Sri Lanka Standards are subject to periodical revision in order to accommodate the progress made by industry. Suggestions for improvement will be recorded and brought to the notice of the Committees to which the revisions are entrusted.

This Standard does not purport to include all the necessary provisions of a contract

© ISO 2013 - All right reserved.

© SLSI 2022

All right reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the SLSI

Sri Lanka Standard
METHOD OF TESTING FOR RUBBER AND PLASTICS FOR POLYMER
DISPERSIONS AND RUBBER LATICES — DETERMINATION OF pH
(First Revision)

NATIONAL FOREWORD

This Standard was approved by the Sectoral Committee on Chemical and Polymer Technology and authorized for adoption and publication as a Sri Lanka Standard by the Council of the Sri Lanka Standards Institution on 2022-10-25

This Sri Lanka Standard was first published in 2006 as an adoption of **ISO 976: 2006**. The text of the above International Standard has been technically revised as **ISO 976: 2013** Rubber and plastics — Polymer dispersions and rubber lattices — Determination of pH. The International Standard **ISO 976: 2013** has been accepted for adoption as the First Revision of SLS 1287.

This Sri Lanka Standard is identical with **ISO 976: 2013** Rubber and plastics — Polymer dispersions and rubber lattices — Determination of pH, published by the International Organization for Standardization (ISO).

ISO 976: 2013 specifies a method for the determination of the pH of polymer dispersions and rubber latices (natural and synthetic) by means of a pH-meter equipped with a combined glass and silver reference electrode.

TERMINOLOGY AND CONVENTIONS

The text of the International Standard has been accepted as suitable for publication, without deviation, as a Sri Lanka Standard. However, certain terminology and conventions are not identical with those used in Sri Lanka Standards. Attention is therefore drawn to the following:

- a) Wherever the words “International Standard” appear referring to a particular Standard they should be interpreted as “Sri Lanka Standard”.
- b) The comma has been used throughout as a decimal marker. In Sri Lanka Standards it is the current practice to use the full point at the base as the decimal marker.
- c) Wherever page numbers are quoted, they are ISO page numbers.

Cross References

International Standard

Corresponding Sri Lanka Standard

ISO 123, Rubber latex — Sampling

SLS 1304 Part 1 Methods of testing of natural rubber latex - Sampling of latex rubber

ISO 3696, Water for analytical laboratory use — Specification and test methods

No corresponding Sri Lanka Standard

ISO 15528, Paints, varnishes and raw materials for paints and varnishes — Sampling

SLS 523 Method of sampling for paints, varnishes and raw materials for paints and varnishes

.....

INTERNATIONAL
STANDARD

ISO
976

Fourth edition
2013-12-01

**Rubber and plastics — Polymer
dispersions and rubber latices —
Determination of pH**

*Caoutchouc et plastiques — Dispersions de polymères et latex de
caoutchouc — Détermination du pH*



Reference number
ISO 976:2013(E)



COPYRIGHT PROTECTED DOCUMENT

© ISO 2013

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Reagents	1
4 Apparatus	2
5 Sampling	2
6 Procedure	2
6.1 General.....	2
6.2 Maintenance of the electrode.....	3
6.3 Calibration of the pH-meter.....	4
6.4 Measurement of the pH of the test sample.....	5
7 Expression of results	6
8 Test report	6
Annex A (informative) Precision	7
Bibliography	9

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 45, *Rubber and rubber products*, Subcommittee SC 3, *Raw materials (including latex) for use in the rubber industry*.

This fourth edition cancels and replaces the third edition (ISO 976:1996), which has been technically revised. It also incorporates the Amendment (ISO 976:1996/Amd.1:2006). The following are the main changes:

- the normative references were updated;
- in (subclause) [4.2](#), the contact details of a provider of combined electrodes were deleted;
- the precision data were updated.

Rubber and plastics — Polymer dispersions and rubber latices — Determination of pH

WARNING — Persons using this International Standard should be familiar with normal laboratory practice. This International Standard does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

1 Scope

This International Standard specifies a method for the determination of the pH of polymer dispersions and rubber latices (natural and synthetic) by means of a pH-meter equipped with a combined glass and silver reference electrode.

The method is also suitable for prevulcanized latex and compounds containing polymer dispersions or rubber latices, including adhesives.

NOTE The accuracy of the method decreases at pH values above 11.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 123, *Rubber latex — Sampling*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 15528, *Paints, varnishes and raw materials for paints and varnishes — Sampling*

3 Reagents

Use commercially available analytical-grade buffer solutions of known pH or, in the absence of commercial buffer solutions, prepare the solutions required (3.1, 3.2 and 3.3) using only reagents of recognized analytical grade and carbon dioxide-free distilled water or water of equivalent purity (grade 3 as defined in ISO 3696).

3.1 Buffer solution, of nominal pH 7.

Dissolve 3,40 g of potassium dihydrogen phosphate ($\text{KH}_2\text{P}_2\text{O}_7$) and 3,55 g of disodium hydrogen phosphate (Na_2HPO_4) in water and make up to 1 000 cm^3 in a volumetric flask.

The pH of this solution is 6,87 at 23 °C.

Store the solution in a glass or polyethylene vessel, which is resistant to chemicals.

3.2 Buffer solution, of pH 4.

Dissolve 10,21 g of potassium hydrogen phthalate ($\text{KOC}_6\text{H}_4\text{COOH}$) in water and make up to 1 000 cm^3 in a volumetric flask.

The pH of this solution is 4,00 at 23 °C.

Store the solution in a glass or polyethylene vessel, which is resistant to chemicals.

3.3 Buffer solution, of nominal pH 9

Dissolve 3,814 g of sodium tetraborate decahydrate ($\text{Na}_2\text{B}_4\text{O}_7 \cdot 10\text{H}_2\text{O}$) in water and make up to 1 000 cm³ in a volumetric flask.

The pH of this solution, when freshly prepared, is 9,20 at 23 °C.

Store the solution in a glass or polyethylene vessel, which is resistant to chemicals, and fitted with a soda-lime carbon dioxide trap. Replace the solution after one month.

Alkaline buffer solutions are unstable; they absorb carbon dioxide from the atmosphere. When an alkaline buffer has been used for calibration, the accuracy can be verified by means of the buffer solution of pH 4.

3.4 Reference electrolyte.

Use 3 mol/dm³ potassium chloride solution saturated with silver chloride.

4 Apparatus

Use usual laboratory equipment and the following.

4.1 pH-meter, with an input impedance of at least 10^{12} Ω, a resolution of 0,01 pH units and equipped for temperature compensation.

4.2 Combined electrode, in which the glass electrode is surrounded concentrically by the silver reference electrode. The reference electrolyte (3.4) is kept in electrical contact with the test sample by a chemically inert diaphragm, e.g. a retractable sleeve made of polytetrafluoroethylene or glass. This is supplied with the electrode by the electrode manufacturer.

A typical combined electrode is shown in [Figure 1](#).

The glass electrode used shall be one recommended by the manufacturer as suitable over the pH range to be encountered (0 to 14 in the case of polychloroprene latices).

Electrical contact between the electrolyte and the test sample is maintained through a thin film of electrolyte between the sleeve and the electrode.

The electrode functions linearly between pH 0 and the appearance of the alkaline error, which, depending on the sodium ion concentration, usually does not appear until the pH is over 11.

4.3 Magnetic stirrer and magnetic bar.

4.4 Electrode holder.

5 Sampling

Carry out the sampling of the rubber latex or polymer dispersion in accordance with one of the methods specified in ISO 123 or ISO 15528.

6 Procedure

6.1 General

In order to reduce thermal and electrical hysteresis effects, ensure that the temperatures of the test samples, electrode, demineralized or distilled rinsing water and buffer solutions are as close to one


another as possible. The temperatures of the test samples and buffer solutions shall not differ by more than 1 °C. The temperature for the determination shall be 23 °C ± 3 °C (27 °C ± 3 °C in tropical countries).

NOTE The pH variation over the range of 20 °C to 30 °C is negligible. In addition, the temperature compensator in the instrument should be set at the actual temperature.

6.2 Maintenance of the electrode

The combined electrode (4.2) shall be maintained following the manufacturer's instructions, paying particular attention to the following points.

- a) Refill the electrode with the reference electrolyte (3.4) through the filling hole, first removing the filling cap if one is fitted. Slightly withdraw the seated sleeve to eliminate any latex deposits and allow a drop of the electrolyte to appear before reseating the sleeve. Prior to calibration and measurement, remove the cap on the electrolyte filling hole to allow the reference electrolyte to be at atmospheric pressure.
- b) When it is not in use, keep the electrode with the junction immersed in the electrolyte.

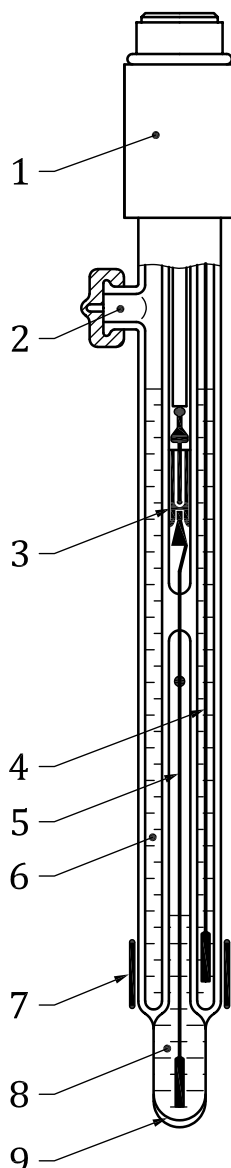

Key

- | | | | |
|---|---------------------|---|---|
| 1 | sliding head | 6 | reference electrolyte (3.4) |
| 2 | filling hole | 7 | seated PTFE or glass diaphragm (sleeve) |
| 3 | connector | 8 | internal buffer |
| 4 | reference electrode | 9 | membrane |
| 5 | internal electrode | | |

Figure 1 — Typical combined electrode

6.3 Calibration of the pH-meter

6.3.1 Switch on the pH-meter (4.1) and allow the electronic circuit to stabilize. Calibrate the pH-meter following the manufacturer's instructions. If not available, proceed as follows.

6.3.2 Select two commercial buffer solutions (see Clause 3), one of nominal pH 7 (i.e. close to the zero point of the electrode) and the other differing from the first by about 3 pH units and of a higher or lower pH corresponding to the sample to be tested. In the event that commercial buffer solutions are not available, use the appropriate prepared buffer solutions (3.1 and 3.2 or 3.3).

6.3.3 Allow the temperature of the buffer solutions, the test sample, and the electrode to equilibrate at the specified temperature (see [6.1](#)). Record the temperature and adjust the temperature correction on the pH-meter to correspond.

6.3.4 Rinse the electrode with distilled or demineralized water (see [Clause 3](#)), and then with the buffer solution of nominal pH 7, so that the liquid runs down the length of the electrode.

6.3.5 Introduce an adequate volume of the same buffer solution into a suitable clean, dry glass or inert plastic vessel. Immerse the electrode in it, taking care that the level of reference electrolyte in the electrode remains about 5 cm higher than the level of the buffer solution to prevent any contamination of the electrode.

Stir gently and allow the reading to stabilize. Adjust the pH-meter using the zero-point adjustment control, so that the reading corresponds to the pH of the buffer solution. Withdraw the electrode and discard the portion of buffer solution.

6.3.6 Rinse the electrode with water, followed by the chosen buffer solution, pH 4 ([3.2](#)) or pH 9 ([3.3](#)), as described in [6.3.4](#).

Instead of the prepared solution of pH 9 ([3.3](#)), commercial buffer solution with a pH in the range 9 to 11 can also be used, if available.

6.3.7 Immerse the electrode in a quantity of the chosen buffer solution as described in [6.3.5](#). Allow the reading to stabilize before adjusting the meter to the pH of the buffer solution, using the gradient adjustment control and without touching the zero-point control.

Ensure that the electrode gradient is in the range -55,6 mV/pH unit to - 61,5 mV/pH unit, i.e. between 95 % and 103 % of the theoretical value (- 58,57 mV/pH unit at 23 °C).

If the electrode is outside this range, carry out the maintenance procedure specified in [6.2](#).

Discard the portion of buffer solution.

6.4 Measurement of the pH of the test sample

6.4.1 Mix the test sample thoroughly to ensure that it is homogeneous.

6.4.2 Rinse the electrode and measuring vessel, first with distilled or demineralized water, and then with some of the sample to be tested, as described in [6.3.4](#). Transfer an adequate volume into the vessel (an additional clean, dry vessel can be used) and immerse the electrode in it as described in [6.3.5](#). Stir gently.

Allow the pH-meter reading to stabilize and record the pH.

Clean the electrode by rinsing with distilled or demineralized water to remove any latex before it dries.

6.4.3 Repeat the operations specified in [6.4.2](#) with a fresh portion of the test sample.

If the new reading does not differ from the first by more than 0,1 pH unit, the determination is complete.

If the two readings differ by more than 0,1 pH unit, make two further determinations, having first carried out all the checks necessary to detect any sources of error.

If a series of consecutive determinations is to be made, recalibrate the pH-meter in accordance with [6.3](#) at 30 min intervals or more frequently depending on the change found at each successive check.

7 Expression of results

Calculate the mean of the two readings that agree and round to the nearest 0,1 of a pH unit.

Express the results in units of pH at 23 °C if the determination was carried out at this temperature. Otherwise, specify the temperature of the determination.

8 Test report

The test report shall contain the following information:

- a) a reference to this International Standard, i.e. ISO 976;
- b) sufficient information to identify the sample;
- c) the pH of the rubber latex or polymer dispersion, expressed to the nearest 0,1 pH unit, and the temperature of the determination;
- d) any particular features noted during the test;
- e) any departure from the procedures specified in this International Standard or the International Standards to which it refers, as well as any operation considered as optional;
- f) the date and the place of the test.

Annex A (informative)

Precision

A.1 General

The precision of this method was determined in accordance with ISO/TR 9272. Make reference to this Technical Report for terminology and explanations of statistical concepts.

The precision details in this precision statement provide an estimate of the precision of this test method with the materials used in the particular interlaboratory programme (ITP) as described below. The precision parameters should not be used for acceptance/rejection testing of any group of materials without documentation that the parameters are applicable to those particular materials and the specific test protocol of this test method.

The precision results are given in [Table A.1](#). The precision is expressed on the basis of a 95 % confidence level for the values established for repeatability, r , and reproducibility, R .

The results in [Table A.1](#) are mean values and give an estimate of the precision of this test method as determined in the ITP conducted in 2011. Sixteen laboratories performed duplicate analyses on two samples, A and B, which were prepared from highly ammoniated latex. The bulk latex was strained and then homogenized by thorough blending and stirring prior to being subsampled into 1-l bottles labelled A and B. Thus, essentially, samples A and B were the same and were treated as such in the statistical computations. Each participating laboratory was required to carry out the test using these two samples on the dates which had been given to the participants in the ITP.

A type 1 precision was determined, based on the sampling method used for the latex samples in the ITP.

A.2 Repeatability

The repeatability, r (in measurement units) of the test method has been established as the appropriate value tabulated in [Table A.1](#). Two single test results, obtained in the same laboratory under normal test method procedures that differ by more than the tabulated, r (for any given level) should be considered to have come from different, or non-identical, sample populations.

A.3 Reproducibility

The reproducibility, R (in measurement units) of the test method has been established as the appropriate value tabulated in [Table A.1](#). Two single test results, obtained in different laboratory under normal test method procedures that differ by more than the tabulated, R (for any given level) should be considered to have come from different, or non-identical, sample populations.

A.4 Bias

In test method terminology, bias is the difference between an average test value and the reference (or true) test property value.

Reference values do not exist for this test method since the value (of the test property) is exclusively defined by the test method. Bias, therefore, cannot be determined for this particular test method.

Table A.1 — Precision data for determination of pH

Mean	Within-laboratory		Between laboratories	
	s_r	r	s_R	R
10,48	0,018	0,05	0,197	0,56
r is the repeatability (in measurement units) s_r is the within-laboratory standard deviation R is the reproducibility (in measurement units) s_R is the between-laboratories standard deviation				

Bibliography

- [1] ISO/TR 9272, *Rubber and rubber products — Determination of precision for test method standards*

SLS CERTIFICATION MARK

The Sri Lanka Standards Institution is the owner of the registered certification mark shown below. Beneath the mark, the number of the Sri Lanka Standard relevant to the product is indicated. This mark may be used only by those who have obtained permits under the SLS certification marks scheme. The presence of this mark on or in relation to a product conveys the assurance that they have been produced to comply with the requirements of the relevant Sri Lanka Standard under a well designed system of quality control inspection and testing operated by the manufacturer and supervised by the SLSI which includes surveillance inspection of the factory, testing of both factory and market samples.

Further particulars of the terms and conditions of the permit may be obtained from the Sri Lanka Standards Institution, 17, Victoria Place, Elvitigala Mawatha, Colombo 08.



SRI LANKA STANDARDS INSTITUTION

The Sri Lanka Standards Institution (SLSI) is the National Standards Organization of Sri Lanka established under the Sri Lanka Standards Institution Act No. 6 of 1984 which repealed and replaced the Bureau of Ceylon Standards Act No. 38 of 1964. The Institution functions under the Ministry of Technology.

The principal objects of the Institution as set out in the Act are to prepare standards and promote their adoption, to provide facilities for examination and testing of products, to operate a Certification Marks Scheme, to certify the quality of products meant for local consumption or exports and to promote standardization and quality control by educational, consultancy and research activity.

The Institution is financed by Government grants, and by the income from the sale of its publications and other services offered for Industry and Business Sector. Financial and administrative control is vested in a Council appointed in accordance with the provisions of the Act.

The development and formulation of National Standards is carried out by Technical Experts and representatives of other interest groups, assisted by the permanent officers of the Institution. These Technical Committees are appointed under the purview of the Sectoral Committees which in turn are appointed by the Council. The Sectoral Committees give the final Technical approval for the Draft National Standards prior to the approval by the Council of the SLSI.

All members of the Technical and Sectoral Committees render their services in an honorary capacity. In this process the Institution endeavours to ensure adequate representation of all view points.

In the International field the Institution represents Sri Lanka in the International Organization for Standardization (ISO), and participates in such fields of standardization as are of special interest to Sri Lanka.