

**SRI LANKA STANDARD 1256: PART 2: 2019**  
**(ISO 2431: 2019)**  
**UDC 667.661**

**METHODS OF TEST FOR  
PAINTS AND VARNISHES  
PART 2: DETERMINATION OF FLOW TIME BY  
THE USE OF FLOW CUPS**  
*(FIRST REVISION)*

**SRI LANKA STANDARDS INSTITUTION**



**Sri Lanka Standard**  
**METHODS OF TEST FOR PAINTS AND VARNISHES**  
**PART 2: DETERMINATION OF FLOW TIME BY THE USE OF FLOW CUPS**  
**(FIRST REVISION)**

**SLS 1256: Part 2: 2019**  
**(ISO 2431: 2019)**

**Gr. H**

*Copyright Reserved*  
**SRI LANKA STANDARDS INSTITUTION**  
**17, Victoria Place**  
**Elvitigala Mawatha**  
**Colombo - 08**  
**Sri Lanka.**

Sri Lanka Standards are subject to periodical revision in order to accommodate the progress made by industry. Suggestions for improvement will be recorded and brought to the notice of the Committees to which the revisions are entrusted.

This Standard does not purport to include all the necessary provisions of a contract

© ISO 2019 - All right reserved.

© SLSI 2019

All right reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the SLSI.

**Sri Lanka Standard**  
**METHODS OF TEST FOR PAINTS AND VARNISHES**  
**PART 2: DETERMINATION OF FLOW TIME BY THE USE OF FLOW CUPS**  
**(FIRST REVISION)**

**NATIONAL FOREWORD**

This Standard was approved by the Sectoral Committee on Chemical and Polymer Technology and authorized for adoption and publication as a Sri Lanka Standard by the Council of the Sri Lanka Standards Institution on 2019-10-22

This Sri Lanka Standard was first published in 2004 which was an adoption of ISO 2431: 1993 Determination of flow time by the use of flow cups. The text of the above International Standard has been technically revised as ISO 2431: 2019 Determination of flow time by the use of flow cups. The International Standard ISO 2431: 2019 has been accepted for adoption as the First Revision of SLS 1256: Part 2; 2019.

This Sri Lanka Standard is identical with ISO 2431: 2019 Paints and varnishes – Determination of flow time by the use of flow cups, published by the International Organization for Standardization (ISO).

**TERMINOLOGY AND CONVENTIONS**

The text of the International Standard has been accepted as suitable for publication, without deviation, as a Sri Lanka Standard. However, certain terminology and conventions are not identical with those used in Sri Lanka Standards. Attention is therefore drawn to the following:

- a) Wherever the words “International Standard” appear referring to a particular Standard they should be interpreted as “Sri Lanka Standard”.
- b) The comma has been used throughout as a decimal marker. In Sri Lanka Standards it is the current practice to use the full point at the base as the decimal marker.
- c) Wherever page numbers are quoted, they are ISO page numbers.

## **Cross References**

### **International Standard**

ISO 1513, Paints and varnishes — Examination and preparation of test samples

ISO 4618, Paints and varnishes – Terms and definitions

ISO 15528, Paints, varnishes and raw materials for paints and varnishes — Sampling

### **Corresponding Sri Lanka Standard**

SLS 1256, Methods of test for paints and varnishes Part 1: Examination and preparation of samples for testing

SLS 1541, Terms and definitions for Paints and varnishes

SLS 523, Methods of sampling for paints, varnishes and raw materials for paints and varnishes

.....

INTERNATIONAL  
STANDARD

SLS 1256 Part 2: 2019

**ISO**  
**2431**

Sixth edition  
2019-06

Corrected version  
2019-09

---

---

**Paints and varnishes — Determination  
of flow time by use of flow cups**

*Peintures et vernis — Détermination du temps d'écoulement au  
moyen de coupes d'écoulement*



Reference number  
ISO 2431:2019(E)

© ISO 2019



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2019

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Fax: +41 22 749 09 47  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland



# Contents

Page

<b>Foreword</b> .....	<b>iv</b>
<b>Introduction</b> .....	<b>v</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Temperature considerations</b> .....	<b>2</b>
<b>5 Apparatus</b> .....	<b>2</b>
5.1 Flow cups.....	2
5.1.1 Dimensions.....	2
5.1.2 Material.....	2
5.1.3 Construction.....	2
5.1.4 Finish.....	3
5.1.5 Measurement range.....	4
5.1.6 Marking.....	5
5.1.7 Care and checking of flow cups.....	5
5.2 Supplementary apparatus.....	6
<b>6 Sampling</b> .....	<b>6</b>
<b>7 Procedure</b> .....	<b>6</b>
7.1 Preliminary check for Newtonian flow.....	6
7.2 Determination of flow time.....	6
7.2.1 Choice of flow cup.....	6
7.2.2 Temperature adjustment.....	6
7.2.3 Preparation of the flow cup.....	7
7.2.4 Filling the flow cup.....	7
7.2.5 Measurement of flow time.....	7
7.2.6 Repeat determinations.....	7
<b>8 Marking of products tested</b> .....	<b>7</b>
<b>9 Precision</b> .....	<b>8</b>
9.1 General.....	8
9.2 Repeatability limit, <i>r</i> .....	8
9.3 Reproducibility limit, <i>R</i> .....	8
<b>10 Test report</b> .....	<b>9</b>
<b>Annex A (normative) Checking flow cups for wear and tear</b> .....	<b>10</b>
<b>Annex B (informative) Conversion of flow times from one temperature to another</b> .....	<b>12</b>
<b>Bibliography</b> .....	<b>14</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 35, *Paints and varnishes*, Subcommittee SC 9, *General test methods for paints and varnishes*.

This sixth edition cancels and replaces the fifth edition (ISO 2431:2011), which has been technically revised. The main changes compared to the previous edition are as follows:

- a general reference to ISO 4618 has been added in [Clause 3](#);
- the information in [Clause 4](#) on measuring at other temperatures and humidities specified in this document has been amended;
- [Figure 1](#) has been corrected;
- information on conduction of measurements in a fume cupboard has been added to [Clause 4](#).

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

This corrected version of ISO 2431:2019 incorporates the following correction:

- In [Table 1](#), the formula for calculating the kinematic viscosity,  $\nu$ , of flow cup No 5 was corrected to

$$\text{read: } \nu = 3,28 \times t - \frac{220}{t}.$$

## Introduction

The first edition of this document, ISO 2431, published in 1972, specified only one flow cup with an orifice diameter of 4 mm. The second edition specified three flow cups with an orifice diameter of 3 mm, 4 mm and 6 mm. The third edition corrected errors in Figures 2 and 4 and the formulae for those figures. The fourth edition specified four flow cups with an orifice diameter of 3 mm, 4 mm, 5 mm and 6 mm. In the fifth edition the curves in Figures 2 to 5 have been placed in a single figure ([Figure 2](#)) and the formulae for the conversion of flow time to kinematic viscosity and vice versa represented by the curves in these figures have been moved from the figures to a table ([Table 1](#)). The procedure for checking the flow cups for wear and tear has been revised to include two alternative methods (one using a certified reference material or secondary working standard, the other using a certified flow cup) and has been moved to an informative annex. The main changes made in this sixth edition are given in the foreword.

As is well known, many countries over the years have developed their own standard flow cups and the difficulty in correlation between them has led to considerable confusion in comparing values. The standardization of an improved design of flow cup has been recommended after careful consideration of the role of flow cups for the measurement of the flow time of paints, varnishes and related products.

Flow times are a measure for sample viscosity only for products with Newtonian or near-Newtonian flow properties. This effectively limits the practical use of flow cups. Nevertheless, for checking purposes, these flow cups do serve a useful purpose. Furthermore, the measurement of flow time is often used to confirm the application consistency.

Paints often contain thickening agents to ensure increased viscosity. Such paints exhibit non-Newtonian flow properties. Their viscosity during application can only be properly assessed using viscometers such as that described in ISO 3219.

Resins and varnishes can exhibit Newtonian or near-Newtonian flow at much higher viscosities than most paints and, where this applies, flow cups can provide a useful means of controlling the consistency. As a result, this document provides flow cups suitable for viscosities up to about 700 mm<sup>2</sup>/s.

With thixotropic materials, stirring or other such mechanical stress immediately before testing will reduce the flow time compared with that for an unstirred sample. With such materials, uncertain and variable flow time values are obtained with all the flow cups. The repeatability and reproducibility limits given in [Clause 9](#) cannot be achieved in the determination of the flow time of such materials.



# Paints and varnishes — Determination of flow time by use of flow cups

## 1 Scope

This document specifies a method for determining the flow time of paints, varnishes and related products that can be used to control consistency.

Four flow cups of similar dimensions, but having orifice diameters of 3 mm, 4 mm, 5 mm and 6 mm, are specified. Two methods for checking the flow cups for wear and tear are given (see [Annex A](#)).

Flow cups with a replaceable jet are not covered by this document as the close tolerances on the supply of the material under test to the jet are not met.

Commonly used dipping flow cups are also not covered by this document.

**NOTE** Since the fabrication tolerances for such flow cups are greater than those of the flow cups specified in this document, flow time determinations with dipping flow cups give a precision which is lower than that obtained with the flow cups specified in this document (see [Clause 9](#)).

The method described in this document is limited to testing materials for which the breakpoint of the flow from the orifice of the flow cup can be determined with certainty. This point is difficult to determine and reproduce for materials with flow times near the upper limit of the measurement range (100 s) due to slowing-down effects.

## 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1513, *Paints and varnishes — Examination and preparation of test samples*

ISO 4618, *Paints and varnishes — Terms and definitions*

ISO 15528, *Paints, varnishes and raw materials for paints and varnishes — Sampling*

## 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 4618 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

— ISO Online browsing platform: available at <https://www.iso.org/obp>

— IEC Electropedia: available at <http://www.electropedia.org/>

### 3.1

#### flow time

*t*

time that elapses from the moment when the material under test starts to flow from the orifice of the filled flow cup to the moment when the flow stream of material first breaks off close to the orifice

### 3.2

#### **Newtonian flow**

behaviour where the shear viscosity is independent of shear rate, shear stress and time

### 3.3

#### **non-Newtonian flow**

behaviour where the shear viscosity is dependent either on shear rate and shear stress or on shear rate, shear stress and time

### 3.4

#### **kinematic viscosity**

$\nu$

ratio of shear viscosity and density

Note 1 to entry: The kinematic viscosity  $\nu$  has the unit square metres per second ( $\text{m}^2\cdot\text{s}^{-1}$ ).

## 4 Temperature considerations

Temperature and humidity are important parameters affecting test results. Deviations from the requirements specified can lead to results that are not comparable. However, the interested parties may agree upon alternative parameters and these parameters shall be reported.

The effect of temperature on flow time is highly significant with respect to application properties and varies with the type of product.

For reference purposes,  $(23,0 \pm 0,5)$  °C is specified as the test temperature in this document. However, it might be more convenient to carry out comparative testing at some other agreed temperature (for example, 25 °C) because of prevailing temperature conditions (see also [Annex B](#)).

For control by flow time, the test sample and flow cup shall be conditioned to an agreed or specified temperature and it shall be ensured that the temperature variation does not exceed 0,5 K during testing. The flow cup shall be in a place which is free from draughts.

If testing is conducted in a fume cupboard and the air suction is left on, this shall be noted in the test report.

## 5 Apparatus

### 5.1 Flow cups

#### 5.1.1 Dimensions

The dimensions of the ISO flow cups and the tolerances allowed in manufacture shall be as shown in [Figure 1](#).

NOTE The most critical tolerance is the internal diameter of the jet of the flow cup, because the flow time is inversely proportional to the fourth power of this dimension.

#### 5.1.2 Material

The jet of the flow cup shall be made of stainless steel or sintered carbide, and the body of the flow cup shall be made of a material which is corrosion-resistant and is not affected by the products to be tested.

#### 5.1.3 Construction

The dimensions not specified, such as wall thickness, shall be such that no distortion of the flow cup can occur in use. The external shape should preferably be as shown in [Figure 1](#), but may be modified for convenience of use, or manufacture, provided that the protruding jet of the flow cup is protected from

accidental damage as far as possible by an external protective sleeve. Such a protective sleeve shall not be immediately adjacent to the jet, so as to prevent any capillary action when the material under test flows out.


Flow cups having an additional jacket for temperature control are preferred.

#### 5.1.4 Finish

The interior surfaces of the flow cups, including the orifice, shall be smooth and free from turning marks, crevices, ledges and burrs which might cause random flow or trap sample or cleaning material.

The standard of finish required is equivalent to a maximum roughness Ra (as defined in ISO 4287) of not more than 0,5 µm.

Dimensions in millimetres  
 Roughness in micrometres

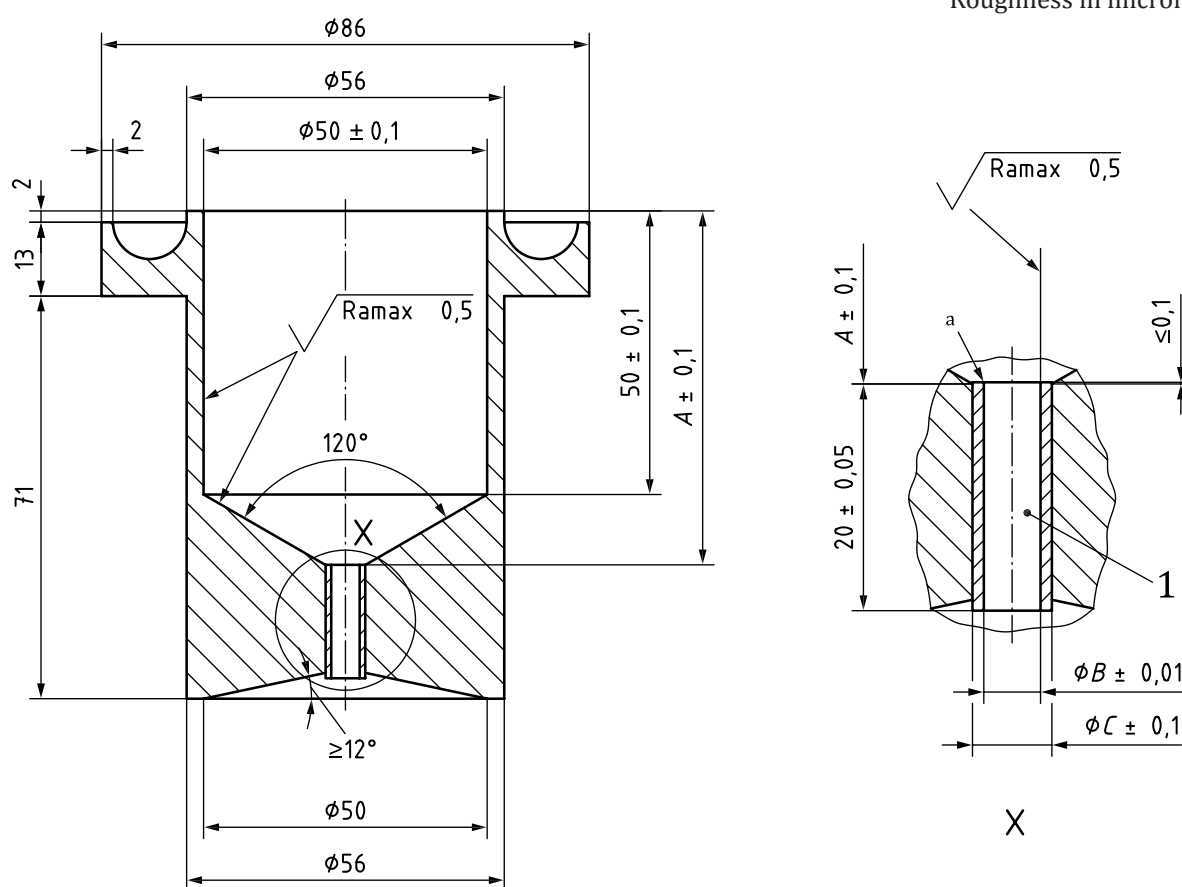

#### Key

- 1 jet
- a Sharp edge (not rounded).

Dimension	Values <sup>b</sup> for the flow cups given			
	3-mm (No 3) flow cup	4-mm (No 4) flow cup	5-mm (No 5) flow cup	6-mm (No 6) flow cup
A	63	62,7	62,4	62,1
B	3	4	5	6
C	5	6	7	8

<sup>b</sup> For tolerances, see the enlarged section of the jet.

Figure 1 — Flow cup

### 5.1.5 Measurement range

Flow cups shall be used within the measurement range given in [Table 1](#). Meaningful data can only be obtained in this range. In addition, the conversion of flow time to kinematic viscosity and *vice versa*, shall be carried out using the formulae given in [Table 1](#).


**Table 1 — Measurement range of flow cups and conversion of flow time to kinematic viscosity and *vice versa***

Flow cup	Flow time, $t$ s	Kinematic viscosity, $\nu$ mm <sup>2</sup> /s	Measurement range s
No 3	$t = \frac{\nu}{0,89} + \sqrt{451,5 + \left(\frac{\nu}{0,89}\right)^2}$	$\nu = 0,443 \times t - \frac{200}{t}$	$30 \leq t \leq 100$
No 4	$t = \frac{\nu}{2,74} + \sqrt{146,0 + \left(\frac{\nu}{2,74}\right)^2}$	$\nu = 1,37 \times t - \frac{200}{t}$	$30 \leq t \leq 100$
No 5	$t = \frac{\nu}{6,56} + \sqrt{67,1 + \left(\frac{\nu}{6,56}\right)^2}$	$\nu = 3,28 \times t - \frac{220}{t}$	$30 \leq t \leq 100$
No 6	$t = \frac{\nu}{13,8} + \sqrt{82,6 + \left(\frac{\nu}{13,8}\right)^2}$	$\nu = 6,90 \times t - \frac{570}{t}$	$30 \leq t \leq 100$

The curves corresponding to the formulae given in [Table 1](#) are plotted in [Figure 2](#).

NOTE These curves are given for information only.



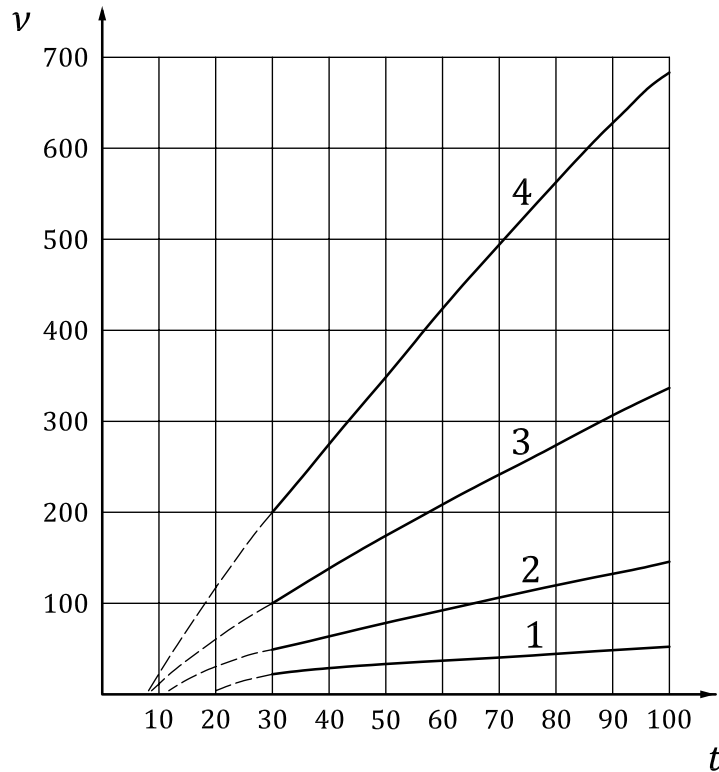

**Key**

- 1 3-mm flow cup
- 2 4-mm flow cup
- 3 5-mm flow cup
- 4 6-mm flow cup
- $t$  flow time, in seconds
- $v$  kinematic viscosity, in square millimetres per second

**Figure 2 — Conversion curves for 3-mm, 4-mm, 5-mm and 6-mm flow cups**

**5.1.6 Marking**

Each flow cup shall have the following inscriptions permanently and legibly marked on it:

- a) designation of flow cup:  
 Flow cup ISO 2431, No 3, No 4, No 5 or No 6;
- b) manufacturer's identification number;
- c) manufacturer's name or trade mark.

**5.1.7 Care and checking of flow cups**

Clean the flow cup immediately after use and before the sample starts to dry, using a suitable solvent. Never use metal tools or a wire scourer for cleaning purposes. If the orifice becomes contaminated with dried deposits, soften these with a suitable solvent and clean carefully, for example with a soft cloth pulled through the orifice.

Check the flow cups periodically for wear and tear using one of the procedures specified in [Annex A](#).

## 5.2 Supplementary apparatus

5.2.1 **Thermometer**, graduated at intervals of 0,2 °C or finer.

5.2.2 **Stand**, suitable for holding the flow cup and provided with levelling screws.

5.2.3 **Spirit level**, preferably of the circular type.

5.2.4 **Flat glass plate with rounded edges** or **straight-edge scraper**.

5.2.5 **Stopwatch**, or other suitable timing-device, with scale divisions of 0,2 s or finer.

5.2.6 **Temperature-controlled room or enclosure**, capable of maintaining the flow cup and sample at a recommended, constant temperature (see [Clause 4](#)).

NOTE This will not be needed if the flow cup has a jacket for temperature control.

## 6 Sampling

Take a representative sample of the material to be tested, as described in ISO 15528. Examine and prepare the sample for testing, as described in ISO 1513.

A sample of 150 ml is sufficient for carrying out one test. Take care to mix the material thoroughly, while at the same time avoiding, as far as possible, loss of solvent by evaporation.

## 7 Procedure

### 7.1 Preliminary check for Newtonian flow

7.1.1 Choose a flow cup that will give a flow time of between 30 s and 100 s for the test material.

7.1.2 Determine the flow time as specified in [7.2](#).

7.1.3 Repeat the determination, but this time allow the material to remain in the flow cup for 60 s before removing the finger used to close off the orifice (see [7.2.4](#)).

7.1.4 If the second result differs from the first result by more than 10 %, the material shall be deemed to be non-Newtonian and therefore unsuitable for consistency control by flow time measurement.

### 7.2 Determination of flow time

#### 7.2.1 Choice of flow cup

Choose a flow cup that will give a flow time of between 30 s and 100 s for the test material.

#### 7.2.2 Temperature adjustment

Adjust the temperature of the sample, and the flow cup, to  $(23,0 \pm 0,5)$  °C, or to an alternative agreed temperature (see [Clause 4](#)).

If the temperature-controlled enclosure ([5.2.6](#)) is used, it is advisable to condition the flow cup and the sample by placing them in the enclosure before use.

The sample shall be considered ready for test immediately after all the air bubbles entrained during the preparation procedure have dispersed. Carry out a final check that the temperature of the sample is within 0,5 K of the agreed test temperature immediately prior to filling the flow cup.

### 7.2.3 Preparation of the flow cup

Place the flow cup on the stand (5.2.2), in a position free from draughts and, by using the spirit level (5.2.3) and adjusting the levelling screws of the stand, ensure that the upper rim of the flow cup is in a horizontal plane.

### 7.2.4 Filling the flow cup

With the orifice closed by a finger, fill the flow cup with the well stirred, bubble-free sample, pouring slowly to avoid the formation of air bubbles. If bubbles are formed, allow them to rise to the surface and remove them.

NOTE If the flow cup has been properly levelled, the sample will overflow evenly over the rim into the gallery.

Remove any meniscus formed either by drawing the straight-edge scraper (see 5.2.4) over the entire rim of the flow cup or by sliding over the rim a flat glass plate with rounded edges so that no air bubbles form between the glass and the surface of the sample, subsequently drawing this plate horizontally across the rim of the flow cup so that, when the plate is removed, the level of the sample coincides with the top rim of the flow cup.

### 7.2.5 Measurement of flow time

Place a suitable receiver under the flow cup so that the distance between the orifice of the flow cup and the surface of the received sample is never less than 100 mm. Remove the finger from the orifice and simultaneously start the timing-device (5.2.5), stopping it as soon as the first break occurs in the stream of sample close to the orifice. Record the rounded flow time to the nearest 0,5 s.

### 7.2.6 Repeat determinations

Carry out a second determination on another portion of the originally prepared sample and check carefully that the temperature of testing is within the prescribed limits. Record the flow time to the nearest 0,5 s. Calculate the mean of the two determinations.

If the two determinations differ by more than 5 %, carry out a third determination. If the third determination and either of the previous determinations do not differ by more than 5 %, discard the outlier. Calculate the result as the mean of the two accepted determinations.

If the third determination does not provide this measure of agreement, the method of test is unlikely to be suitable because of non-Newtonian flow behaviour, and consideration shall be given to other methods of test, e.g. to measuring the viscosity using a rotational viscometer.

## 8 Marking of products tested

The product tested may be marked with a marking indicating the results of the test.

If such a marking is made, it shall comprise a reference to this document, the designation number of the flow cup used and the flow time, in seconds. For example,

ISO 2431 – 5 – 65

where

- ISO 2431 is the number of this document;
- 5 is the designation number of the flow cup used;
- 65 is the flow time, in seconds.

## 9 Precision

### 9.1 General

An interlaboratory test was planned and executed, and the results evaluated, in accordance with ISO 5725-2. 11 laboratories participated in the test. Liquids were tested using 4 mm and 6 mm flow cups. Except for the varnish when tested using the 6 mm flow cup, the liquids showed Newtonian flow behaviour. The flow behaviour of the varnish when tested using the 6 mm flow cup was nearly Newtonian, but, when the preliminary check specified in 7.1 was carried out, the second result did not differ from the first result by more than 10 % (see 7.1.4).

### 9.2 Repeatability limit, $r$

The value below which the absolute difference between two single test results, each the mean of duplicates, obtained on identical material by one operator in one laboratory within a short interval of time using the standardized test method, might be expected to lie with a 95 % probability is approximately 2 s.

Details of the results are given in [Table 2](#).

**Table 2 — Repeatability limit,  $r$**

Test liquid	Orifice diameter mm	Mean value of flow time s	Repeatability limit $r$ s
Engine oil	4	55	1,7
Varnish, based on organic solvents	4	56	1,7
Engine oil	6	60	2,6
Varnish, based on organic solvents	6	43	1,7

### 9.3 Reproducibility limit, $R$

The value below which the absolute difference between two single test results, each the mean of duplicates, obtained by operators on identical material in different laboratories using the standardized test method, might be expected to lie with a 95 % probability is approximately 3 s for the 4 mm flow cup and approximately 6 s for the 6 mm flow cup.

Details of the results are given in [Table 3](#).

**Table 3 — Reproducibility limit, *R***

Test liquid	Orifice diameter	Mean value of flow time	Reproducibility limit
	mm	s	<i>R</i> s
Engine oil	4	55	2,2
Varnish, based on organic solvents	4	56	3,2
Engine oil	6	60	3,9
Varnish, based on organic solvents	6	43	5,5

## 10 Test report

The test report shall include at least the following information:

- a) all details necessary to identify the product tested;
- b) a reference to this document (ISO 2431:2019) and to the designation (No 3, No 4, No 5 or No 6) of the flow cup used;
- c) the manufacturer's identification number of the flow cup used;
- d) the temperature of testing;
- e) the flow time (for referee purposes, individual values shall also be reported);
- f) any deviation, by agreement or otherwise, from the test procedure described;
- g) any unusual features (anomalies) observed during the test;
- h) the date of the test.

## Annex A (normative)

### Checking flow cups for wear and tear

#### A.1 General

To monitor wear and tear, flow cups should be checked regularly with one of the two methods in defined intervals, e.g. every six months. In method A, the flow cup is checked by using a certified reference material (CRM) or reference material (RM) (see ISO Guide 30). In method B, the flow cup is checked against a certified flow cup.

#### A.2 Standards required

**A.2.1 Certified Reference Material (CRM)**, comprising a standard Newtonian oil of known kinematic viscosity and known shelf life.

**A.2.2 Reference Material (RM)**, comprising e.g. a commercially available engine oil or other substance with a kinematic viscosity determined by testing representative subsamples at least three times, utilizing an instrument previously verified using a CRM, statistically analysing the results and, after the removal of any outliers, calculating the arithmetic mean of the results.

Store RMs in containers which will retain the integrity of the RM, out of direct sunlight, at a temperature not exceeding 10 °C.

An RM may be used up to three times. It shall then be tempered and allow to stand for devolatilization for at least 3 h.

**A.2.3 Flow cup**, certified.

#### A.3 Method A — Checking using a CRM or RM

To check a particular flow cup, use a CRM or an RM of known kinematic viscosity at  $(23 \pm 0,2)$  °C. Choose a CRM or RM with a flow time which is in the range 30 s to 100 s, and preferably near the midpoint of this range, for the flow cup concerned.

Condition the CRM or RM, and the flow cup being checked, at  $(23 \pm 0,2)$  °C for at least 2 h. Determine the flow time of the CRM or RM, following the procedure specified in [Clause 7](#), to the nearest 0,2 s.

Carry out the determination three times.

Calculate the mean value of the three determinations and, using the appropriate formula in [Table 1](#), the kinematic viscosity of the liquid as given by the flow cup.

Calculate the deviation between the certified and the measured viscosity using [Formula \(A.1\)](#):

$$\Delta v = \frac{(v_m - v_{ce}) \times 100}{v_{ce}} \quad (\text{A.1})$$

where

$\Delta v$  is the deviation between the certified and the measured viscosity, expressed as a percentage;

$v_m$  is the viscosity calculated from the flow time measured, in square millimetres per second;

$v_{ce}$  is the viscosity of the CRM or RM, in square millimetres per second.

If the two values of the calculated kinematic viscosity obtained do not differ by more than 3 %, the flow cup is deemed to be satisfactory for use.

NOTE When using an RM, instead of calculating the kinematic viscosity the flow times measured can be used directly to calculate the deviation, expressed as  $\Delta t$  [see [Formula \(A.2\)](#)].

#### A.4 Method B — Checking using a certified flow cup

To check a particular flow cup, use a certified reference flow cup of the same type. Choose an RM with a flow time which is in the range 30 s to 100 s, and preferably near the midpoint of this range, for the flow cup concerned.

Condition the certified reference flow cup, the flow cup being checked and the RM in a temperature-controlled enclosure at a temperature between 20 °C and 25 °C for at least 2 h. During this conditioning and the subsequent flow time measurement, the temperature shall remain constant to within  $\pm 0,2$  °C. Determine the flow time of the RM, following the procedure specified in [Clause 7](#), to the nearest 0,2 s.

Carry out the determination three times. Calculate the result as the mean of the three determinations.

Calculate the deviation between the flow time given by the certified reference flow cup and that given by the flow cup being checked, using [Formula \(A.2\)](#):

$$\Delta t = \frac{(t_{ch} - t_{ce}) \times 100}{t_{ce}} \quad (\text{A.2})$$

where

$\Delta t$  is the deviation between the flow time given by the certified flow cup and that given by the flow cup being checked, expressed as a percentage;

$t_{ch}$  is the flow time determined with the flow cup being checked, in seconds;

$t_{ce}$  is the flow time determined with the certified reference flow cup, in seconds.

If the two values of the determined flow times obtained do not differ by more than 3 %, the flow cup is deemed to be satisfactory for use.

## Annex B (informative)

### Conversion of flow times from one temperature to another

If the flow time cannot be measured at the specified temperature, it is necessary to convert it from the measurement temperature. This annex describes an interpolation method for the conversion. The method is not suitable for the extrapolation of data outside the defined temperature range.

Vogel's equation is a well-proven and frequently used approximation of the viscosity/temperature behaviour of paints. It is given, for flow times, by [Formula \(B.1\)](#):

$$\ln t = A + \frac{B}{T + C} \quad (\text{B.1})$$

in which the constants  $A$ ,  $B$  and  $C$  are given by [Formula \(B.2\)](#) to [\(B.4\)](#):

$$C = \frac{(\ln t_1 - \ln t_3)(T_1 - T_2)T_3 - (\ln t_1 - \ln t_2)(T_1 - T_3)T_2}{(\ln t_1 - \ln t_2)(T_1 - T_3) - (\ln t_1 - \ln t_3)(T_1 - T_2)} \quad (\text{B.2})$$

$$A = \frac{(T_1 + C)\ln t_1 - (T_2 + C)\ln t_2}{(T_1 - T_2)} \quad (\text{B.3})$$

$$B = (T_2 + C)(\ln t_2 - A) \quad (\text{B.4})$$

where

- $T$  is the temperature, in degrees Celsius;
- $T_1$  is the lower temperature limit, in degrees Celsius;
- $T_2$  is the temperature in the middle of the range, in degrees Celsius;
- $T_3$  is the upper temperature limit, in degrees Celsius;
- $t_1$  is the flow time, in seconds, at temperature  $T_1$ ;
- $t_2$  is the flow time, in seconds, at temperature  $T_2$ ;
- $t_3$  is the flow time, in seconds, at temperature  $T_3$ .

The conversion of flow times from one temperature to another only gives reliable results if

- the chosen temperature range  $T_3 - T_1$  is  $\leq 20$  °C;
- the conversion does not involve extrapolation outside the defined temperature range.

If the constants  $A$ ,  $B$  and  $C$  are known (for an example, see [Table B.1](#)), the interpolation data within the interval from  $T_1$  to  $T_3$  can be calculated using [Formula \(B.1\)](#) and tabulated (for an example, see [Table B.2](#)). Additionally, the data can be plotted as an interpolation curve (for an example, see [Figure B.1](#)).

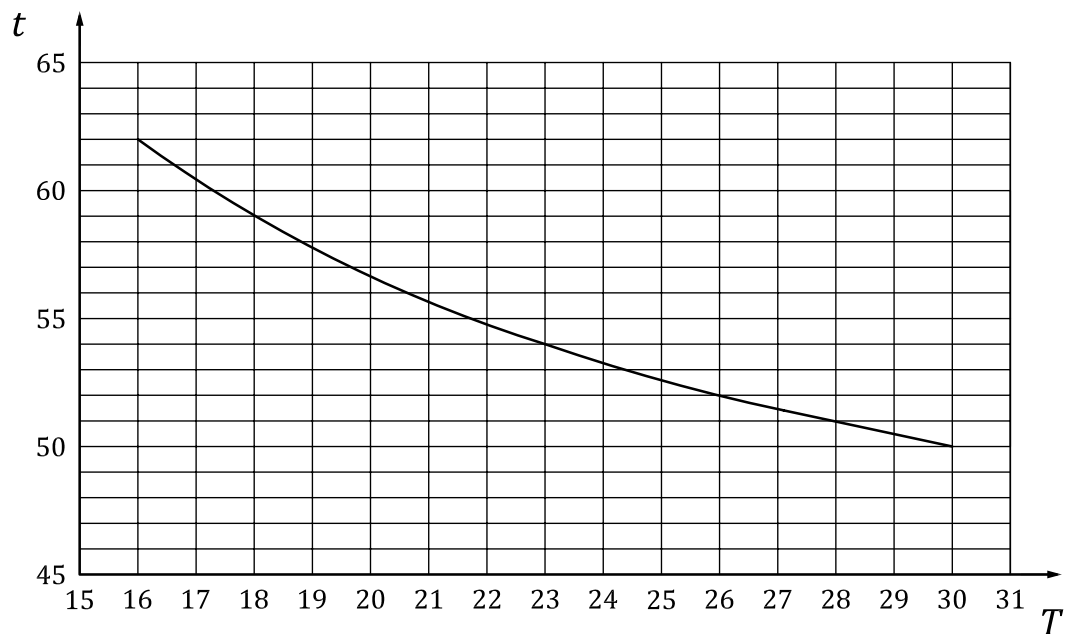


**Table B.1 — Calculation of the constants  $A$ ,  $B$  and  $C$**

Temperature °C		Flow time s		Calculated values of $A$ , $B$ and $C$	
$T_1$	16	$t_1$	62	$A$	3,641
$T_2$	23	$t_2$	54	$B$	8,552
$T_3$	30	$t_3$	50	$C$	1,609

**Table B.2 — Interpolated values of flow time between the three base values**

Temperature °C	Flow time s
16	62,0
17	60,4
18	59,0
19	57,8
20	56,7
21	55,7
22	54,8
23	54,0
24	53,3
25	52,6
26	52,0
27	51,4
28	50,9
29	50,4
30	50,0



**Key**

- $t$  flow time, in seconds
- $T$  temperature, in degrees Celsius

**Figure B.1 — Example of relationship between flow-time  $t$  and temperature  $T$**

## Bibliography

- [1] ISO 3219, *Plastics — Polymers/resins in the liquid state or as emulsions or dispersions — Determination of viscosity using a rotational viscometer with defined shear rate*
- [2] ISO 4287, *Geometrical Product Specifications (GPS) — Surface texture: Profile method — Terms, definitions and surface texture parameters*
- [3] ISO 5725-2, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*
- [4] ISO Guide 30, *Reference materials — Selected terms and definitions*





## **SLS CERTIFICATION MARK**

*The Sri Lanka Standards Institution is the owner of the registered certification mark shown below. Beneath the mark, the number of the Sri Lanka Standard relevant to the product is indicated. This mark may be used only by those who have obtained permits under the SLS certification marks scheme. The presence of this mark on or in relation to a product conveys the assurance that they have been produced to comply with the requirements of the relevant Sri Lanka Standard under a well designed system of quality control inspection and testing operated by the manufacturer and supervised by the SLSI which includes surveillance inspection of the factory, testing of both factory and market samples.*

*Further particulars of the terms and conditions of the permit may be obtained from the Sri Lanka Standards Institution, 17, Victoria Place, Elvitigala Mawatha, Colombo 08.*



## **SRI LANKA STANDARDS INSTITUTION**

The Sri Lanka Standards Institution (SLSI) is the National Standards Organization of Sri Lanka established under the Sri Lanka Standards Institution Act No. 6 of 1984 which repealed and replaced the Bureau of Ceylon Standards Act No. 38 of 1964. The Institution functions under the Ministry of Science & Technology.

The principal objects of the Institution as set out in the Act are to prepare standards and promote their adoption, to provide facilities for examination and testing of products, to operate a Certification Marks Scheme, to certify the quality of products meant for local consumption or exports and to promote standardization and quality control by educational, consultancy and research activity.

The Institution is financed by Government grants, and by the income from the sale of its publications and other services offered for Industry and Business Sector. Financial and administrative control is vested in a Council appointed in accordance with the provisions of the Act.

The development and formulation of National Standards is carried out by Technical Experts and representatives of other interest groups, assisted by the permanent officers of the Institution. These Technical Committees are appointed under the purview of the Sectoral Committees which in turn are appointed by the Council. The Sectoral Committees give the final Technical approval for the Draft National Standards prior to the approval by the Council of the SLSI.

All members of the Technical and Sectoral Committees render their services in an honorary capacity. In this process the Institution endeavours to ensure adequate representation of all view points.

In the International field the Institution represents Sri Lanka in the International Organization for Standardization (ISO), and participates in such fields of standardization as are of special interest to Sri Lanka.